


=====
Acq. Operator : Anderson
Acq. Instrument : Instrument 1 Location : Vial 1
Injection Date : 10/03/2026 16:12:16 Inj : 1
Inj Volume : Manually
Acq. Method : C:\CHEM32\1\2026ATUAL.M\2026PROCE.M
Last changed : 10/03/2026 15:17:30 by Anderson
(modified after loading)
Analysis Method : C:\CHEM32\1\2026ATUAL.M\2026PROCE.M
Last changed : 10/03/2026 17:41:33 by Anderson
Sample Info : SDP 218/26 DILUENTE VITRAN

Sample-related custom fields:

Name	Value
------	-------

Additional Info : Peak(s) manually integrated

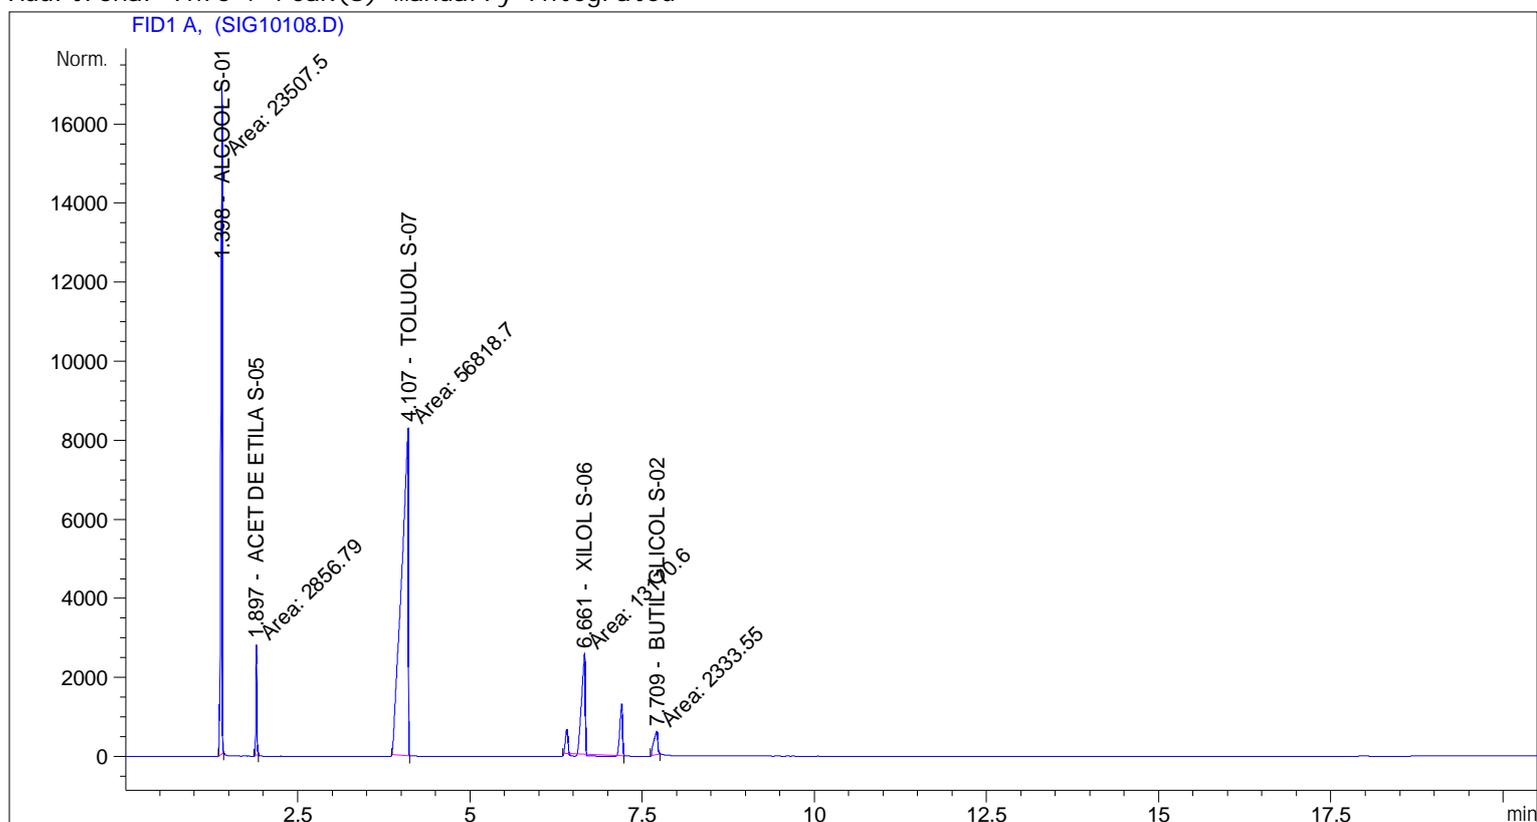

=====
Area Percent Report
=====

Sorted By : Signal
Calib. Data Modified : 10/03/2026 13:10:07
Multiplier : 1.0000
Dilution : 1.0000
Use Multiplier & Dilution Factor with ISTDs

Signal 1: FID1 A,

Peak #	RetTime [min]	Type	Width [min]	Area [pA*s]	Area %	Name
1	0.000		0.0000	0.00000	0.00000	DOWANOL PM S-24
2	1.398	MM T	0.0230	2.35075e4	23.82019	ALCOOL S-01
3	1.433		0.0000	0.00000	0.00000	ACETONA S-08
4	1.500		0.0000	0.00000	0.00000	ACETONA S-08
5	1.515		0.0000	0.00000	0.00000	ISOPROPANOL S-18
6	1.750		0.0000	0.00000	0.00000	HEXANO S-96
7	1.810		0.0000	0.00000	0.00000	MEK S-09
8	1.897	MM T	0.0169	2856.79321	2.89480	ACET DE ETILA S-05
9	2.120		0.0000	0.00000	0.00000	ISOBUTANOL S-20
10	3.200		0.0000	0.00000	0.00000	ETIL GLICOL S-17
11	3.450		0.0000	0.00000	0.00000	MIBK S-16
12	4.107	MM T	0.1141	5.68187e4	57.57458	TOLUOL S-07
13	4.190		0.0000	0.00000	0.00000	TOLUOL S-07
14	5.530		0.0000	0.00000	0.00000	ACETATO DE BUTILA S-32
15	6.200		0.0000	0.00000	0.00000	DIACETONA ALCOOL S-31
16	6.661	MM T	0.0863	1.31706e4	13.34583	XILOL S-06
17	7.010		0.0000	0.00000	0.00000	ACETAMILA S-15
18	7.709	MM T	0.0663	2333.55078	2.36460	BUTIL GLICOL S-02
19	8.100		0.0000	0.00000	0.00000	ACET ETIL GLICOL S-34
20	9.562		0.0000	0.00000	0.00000	AB9 S-12

Totals : 9.86871e4

7 Warnings or Errors :

Warning : Calibration warnings (see calibration table listing)

Warning : Calibrated compound(s) not found

Warning : Invalid calibration curve, (ALCOOL S-01)

Warning : Invalid calibration curve, (ACET DE ETILA S-05)

Warning : Invalid calibration curve, (TOLUOL S-07)

Warning : Invalid calibration curve, (XILOL S-06)

Warning : Invalid calibration curve, (BUTIL GLICOL S-02)

=====
*** End of Report ***