


=====
Acq. Operator : Anderson
Acq. Instrument : Instrument 1 Location : Vial 1
Injection Date : 11/03/2026 15:03:13 Inj : 1
Inj Volume : Manually
Acq. Method : C:\CHEM32\1\2026ATUAL.M\2026PROCE.M
Last changed : 11/03/2026 14:53:27 by Anderson
(modified after loading)
Analysis Method : C:\CHEM32\1\2026ATUAL.M\2026PROCE.M
Last changed : 12/03/2026 08:55:38 by Anderson
(modified after loading)
Sample Info : SDP 222/26 THINNER LIMPEZA VETORE

Sample-related custom fields:

Name	Value
----- -----	
Additional Info : Peak(s) manually integrated	

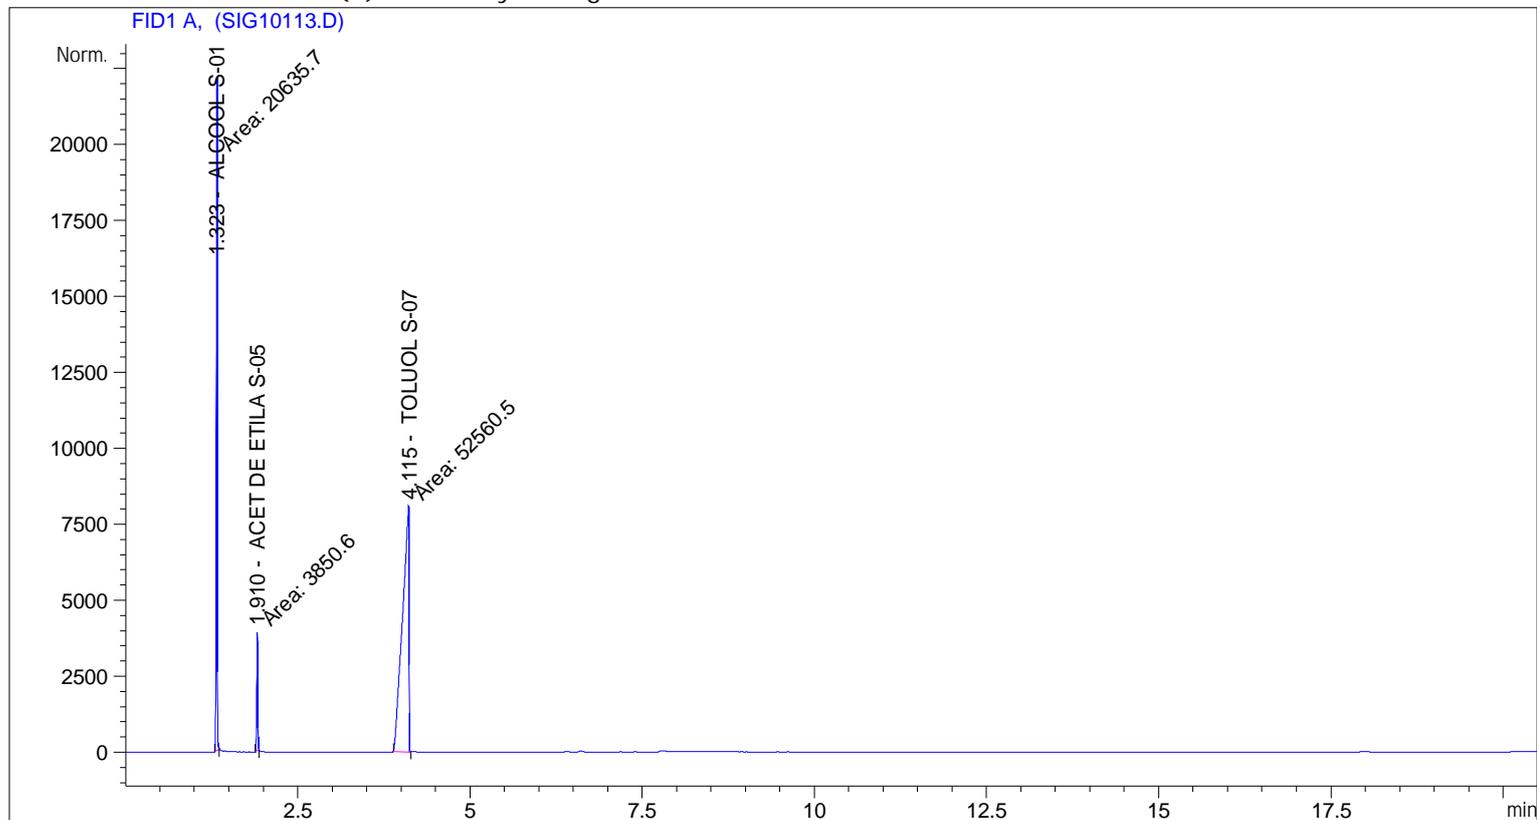

=====
Area Percent Report
=====

Sorted By : Signal
Calib. Data Modified : 12/03/2026 08:55:48
Multiplier : 1.0000
Dilution : 1.0000
Use Multiplier & Dilution Factor with ISTDs

Signal 1: FID1 A,

Peak #	RetTime [min]	Type	Width [min]	Area [pA*s]	Area %	Name
1	0.000		0.0000	0.00000	0.00000	DOWANOL PM S-24
2	1.323	MM T	0.0153	2.06357e4	26.78334	ALCOOL S-01
3	1.412		0.0000	0.00000	0.00000	ALCOOL S-01
4	1.433		0.0000	0.00000	0.00000	ACETONA S-08
5	1.480		0.0000	0.00000	0.00000	ACETONA S-08
6	1.515		0.0000	0.00000	0.00000	ISOPROPANOL S-18
7	1.750		0.0000	0.00000	0.00000	HEXANO S-96
8	1.810		0.0000	0.00000	0.00000	MEK S-09
9	1.910	MM T	0.0163	3850.60498	4.99775	ACET DE ETILA S-05
10	2.120		0.0000	0.00000	0.00000	ISOBUTANOL S-20
11	3.200		0.0000	0.00000	0.00000	ETIL GLICOL S-17
12	3.450		0.0000	0.00000	0.00000	MIBK S-16
13	4.115	MM T	0.1078	5.25605e4	68.21891	TOLUOL S-07
14	4.190		0.0000	0.00000	0.00000	TOLUOL S-07
15	5.530		0.0000	0.00000	0.00000	ACETATO DE BUTILA S-32
16	6.200		0.0000	0.00000	0.00000	DIACETONA ALCOOL S-31
17	6.760		0.0000	0.00000	0.00000	XILOL S-06
18	7.010		0.0000	0.00000	0.00000	ACETAMILA S-15
19	7.900		0.0000	0.00000	0.00000	BUTIL GLICOL S-02
20	8.100		0.0000	0.00000	0.00000	ACET ETIL GLICOL S-34
21	9.562		0.0000	0.00000	0.00000	AB9 S-12

Totals : 7.70468e4

5 Warnings or Errors :

Warning : Calibration warnings (see calibration table listing)

Warning : Calibrated compound(s) not found

Warning : Invalid calibration curve, (ALCOOL S-01)

Warning : Invalid calibration curve, (ACET DE ETILA S-05)

Warning : Invalid calibration curve, (TOLUOL S-07)

=====
*** End of Report ***